

## Series *HEC*

Water-cooled

Can control the temperature of the heat source by using the external temperature sensor (sold separately). (Automatically adjusts to the effects of ambient temperature.)


- ±0.01°C to 0.03°C**

The image displays three pieces of laboratory equipment. On the left is a white, boxy unit labeled 'Water-cooled' with a digital display and control buttons. In the center is a taller, grey and white unit labeled 'Air-cooled' with a large control knob and a digital display. On the right is another tall, grey and white unit labeled 'Water-cooled' with a control knob and a digital display. All three units have a vertical handle on the front and a power cord on the side.

140W: W184 x H262 x D321  
320W: W184 x H262 x D321  
230W: W210 x H393 x D436  
600W: W240 x H390 x D455  
600W: W240 x H390 x D455  
1200W: W300 x H448 x D528


**Air-cooled** | **Series HEC-A**

- **Air-cooled:** Can be used in the environments with no cooling equipment.
- **Cooling capacity:** 230 W, 600 W

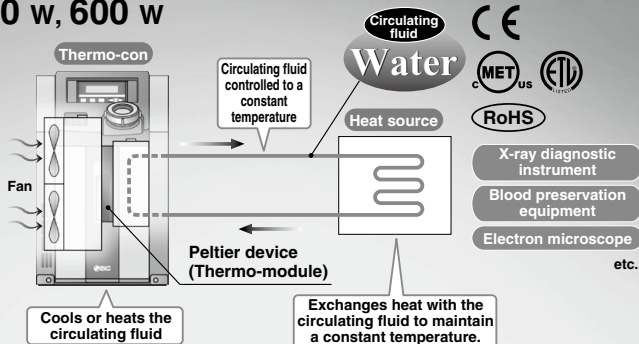

**Water-cooled** *Series HEC-W*

- **Water-cooled:** Can be used in the environments with facility water equipment.
- **Cooling capacity:** 140 W, 320 W, 600 W, 1200 W

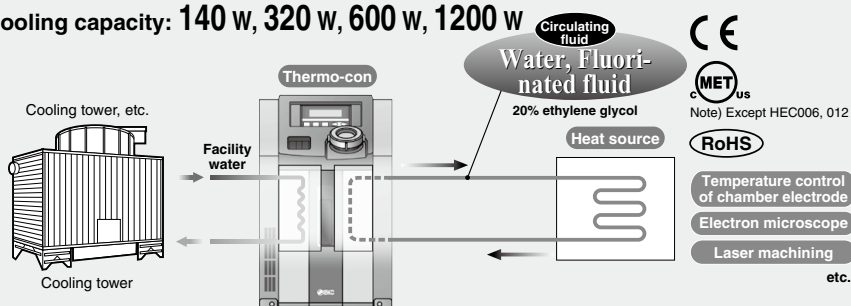

- **Compliant with safety standard for medical equipment IEC 60601-1 (Air-cooled/HEC002-A series)**
- **Power supply: Applicable to 100 V to 240 V**  
(Air-cooled/HEC-A series, Water-cooled/HEC001-W, HEC003-W)
- **Suitable to fluorinated fluids (Fluorinert™ FC-3283, GALDEN® HT135)**  
(Water-cooled/HEC006-W, HEC012-W)
- **Compatible with ethylene glycol 20% (Water-cooled/HEC001-W, HEC003-W)**

### Learning Control Function (Temp. control by external temperature sensor)



This function adjusts the fluid temperature to the set value with an automatic offset setting. Set the external temperature sensor at the circulating fluid inlet located just in front of the heat source, which allows the Thermo-con to sample the fluid temperature. This function is effective when automatically adjusting for heat exhaust from piping, etc. If the external temperature sensor is installed directly on the heat source, the learning control function may not work properly due to large heat volume or large temperature difference. Be sure to install the sensor at the circulating fluid inlet.

## Principle of Peltier Device (Thermo-module)

A Peltier device (thermo-module) is a plate type element, inside which P-type semiconductors and N-type semiconductors are located alternately. If direct current is supplied to the Peltier device (thermo-module), heat is transferred inside the device, and one face generates heat and increases temperature while the other face absorbs heat and decreases temperature. Therefore, changing the direction of the current supplied to the Peltier device (thermo-module) can achieve heating and cooling operation. This method has a fast response and can shift quickly between heating and cooling and so temperature can be controlled very precisely.



### Air-cooled

#### Series HEC-A

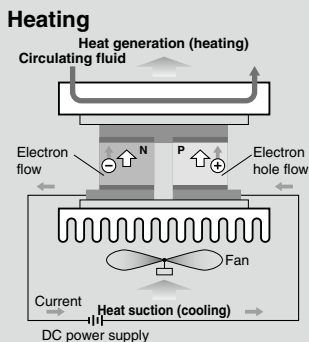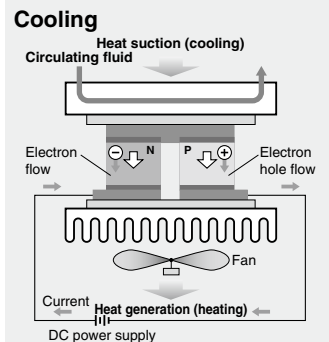

### Water-cooled


#### Series HEC-W

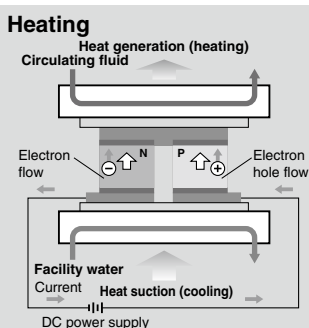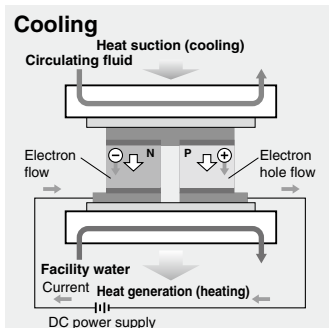

# Construction and Principles


## Air-cooled

## Series HEC-A

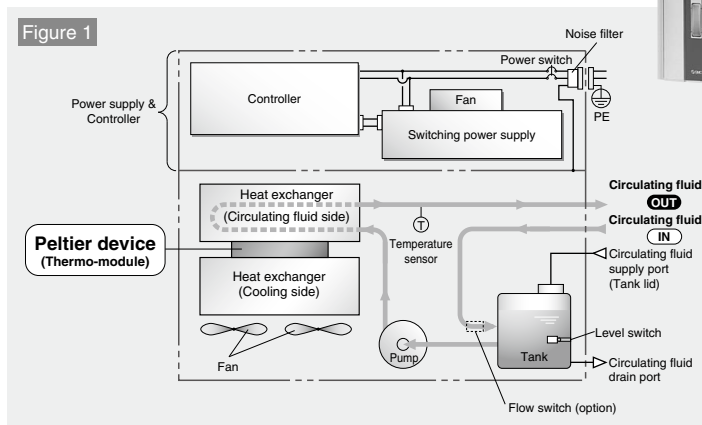


## Water-cooled

## Series HEC-W

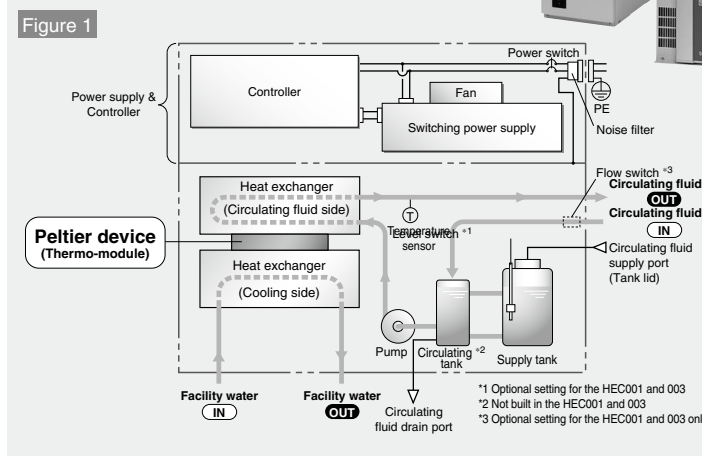

**Figure 2** Example of circulating fluid piping

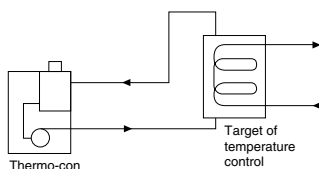

The Thermo-con is constructed as shown in Figure 1. It interposes a Peltier device (thermo-module) between the heat exchangers for the circulating fluid and facility water and controls the pulse width of supply direct current to achieve the target outlet temperature of circulating fluid precisely.

The circulating fluid returns to the tank, and is transferred by the pump which is built in the Thermo-con, and goes through the heat exchangers and internal sensors and out from the circulating fluid outlet.

Figure 2 shows an example of circulating fluid piping. The circulating fluid is transferred at a constant temperature by the pump.

HRG  
 HRS  
 HRZ  
 HRZD  
 HRW  
**HEC**  
 HEB  
 HED  
 HEA  
 IDH

## When to Use Air-Cooled and Water-Cooled Thermo-con

Both air-cooled and water-cooled Thermo-cons are available. Select a proper Thermo-con by referring to the following.

### Air-cooled

- No facility water equipment → Can install the unit easily without facility water equipment.
- Frequent piping changes → Can reduce the piping installation labor since facility water piping is not required.


### Water-cooled

- Need to avoid effects of ambient temperature. → Since the unit is water-cooled, the ambient temperature will have little effect.
- Want to reduce the installation space. → Can reduce the space since the unit is compact.

## Application Examples

### Semiconductor


Example: Temperature control of a chamber electrode

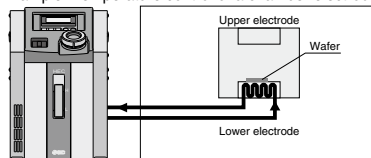

- Etching equipment
- Spatter equipment
- Cleaning equipment
- Coating equipment
- Dicing equipment
- Tester, etc.

### Medical


Example: Blood preservation

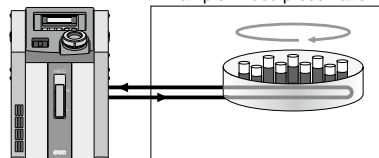

- X-ray diagnostic instrument
- MRI
- Blood preservation equipment

### Machine tool

Example: Laser machining

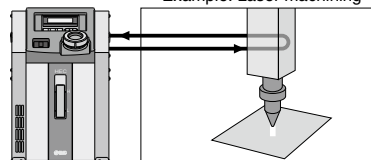


- Wire cutting
- Grinder
- Spot welding
- Plasma welding
- Laser machining, etc.

Temperature-controlling the laser generating tube enables the laser wavelength to be optimised, improving the accuracy of the machined cross sectional area.

### Analysis

Example: Electronic microscope

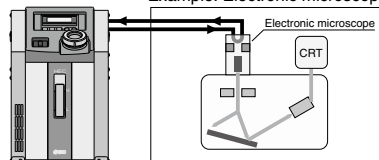

- Electron microscope
- X-ray analytical instrument
- Gas chromatography
- Sugar level analytical instrument, etc.

Prevents the distortion caused by the heat generated by the electronic gun in an electronic microscope.

**Bonding of DVD including next generation**

Air-cooled Water-cooled

**Cooling of semiconductor laser**

Air-cooled Water-cooled

**Temperature control of die-cast mold**

Air-cooled Water-cooled

# CONTENTS

- Features ..... Page 1380 to 1382
- Model Selection ..... Page 1384, 1385



## Air-cooled

### Series **HEC-A**

- How to Order/Specifications ..... Page 1386
- Cooling Capacity/Heating Capacity/  
Pump Capacity (Thermo-con Outlet) ..... Page 1387
- Parts Description ..... Page 1388
- Dimensions ..... Page 1389, 1390
- Connectors ..... Page 1391
- Alarm/Maintenance ..... Page 1392
- Options ..... Page 1393
- Specific Product Precautions ..... Page 1394 to 1396



## Water-cooled Series **HEC-W**

- How to Order/Specifications ..... Page 1398, 1399
- Cooling Capacity/Heating Capacity/  
Pump Capacity (Thermo-con Outlet)/  
Pressure Loss in Facility Water Circuit ..... Page 1400 to 1402
- Parts Description ..... Page 1403
- Dimensions ..... Page 1404 to 1406
- Connectors ..... Page 1407
- Alarm/Maintenance ..... Page 1408
- Options ..... Page 1409
- Specific Product Precautions ..... Page 1410, 1411

HRG

HRS

HRZ

HRZD

HRW

**HEC**

HEB

HED

HEA

IDH

# Series HEC

## Model Selection

### Guide to Model Selection

#### 1. What radiation method will be used?

Without a cooling tower ..... Air-cooled HEC-A series

With a cooling tower ..... Water-cooled HEC-W series

When to Use Air-cooled and Water-cooled Thermo-con

##### <Air-cooled>

- No facility water equipment → Can install the unit easily without facility water equipment.
- Frequent piping changes → Can reduce the piping installation labor since facility water piping is not required.

##### <Water-cooled>

- Need to avoid effects of ambient temperature. → Since the unit is water-cooled, the ambient temperature will have little effect.
- Want to reduce installation space. → Can reduce the space since the unit is compact.

#### 2. How much is the temperature in degrees centigrade for the circulating fluid?

Temperature range which can be set with the Thermo-con: 10 to 60°C

If a lower temperature (down to -20°C) or higher temperature (up to 90°C) than this range is necessary, select the Thermo-chiller HRZ series.

#### 3. What kind of the circulating fluids will be used?

Circulating fluids that can be used in the Thermo-con

Model	Clear water	Fluorinert™ FC-3238 GALDEN® HT135	20% ethylene glycol
HEC001-W, HEC003-W	○	×	○
HEC006-W, HEC012-W	○	○	×
HEC002-A, HEC006-A	○	×	×

○ : Usable    × : Unusable

#### 4. How much cooling capacity required?

Allows a safety factor of 20% over the capacity that is actually required, taking into account the changes in the operating conditions. If a larger capacity than this Thermo-con is necessary, select the Thermo-cooler HRG series or Thermo-chiller HRZ series.

**Example 1** When the heat generation amount in the customer's machine is known.

Heat generation amount: 400 W

Cooling capacity = Considering a safety factor of 20%,  $400 \times 1.2 = 480 \text{ W}$

## Guide to Model Selection

### Example 2 When the heat generation amount in the customer's machine is not known.

Obtain the temperature difference between inlet and outlet by circulating the fluid inside the customer's machine.


Heat generation amount **Q** : Unknown  
 Circulating fluid temperature difference  $\Delta T (= T_2 - T_1)$  : 0.8°C (0.8 K)  
 Circulating fluid outlet temperature **T1** : 25°C (298.15 K)  
 Circulating fluid return temperature **T2** : 25.8°C (298.95 K)  
 Circulating fluid flow rate **L** : 3 L/min  
 Circulating fluid : Water  
 Density  $\gamma$ :  $1 \times 10^3 \text{ kg/m}^3$   
 Specific heat **C**:  $4.2 \times 10^3 \text{ J/(kg} \cdot \text{K)}$

$$Q = \frac{\Delta T \times L \times \gamma \times C}{60 \times 1000}$$

$$= \frac{0.8 \times 3 \times 1 \times 10^3 \times 4.2 \times 10^3}{60 \times 1000}$$

$$= 167 \text{ W}$$

Cooling capacity = Considering a safety factor of 20%,  
 $167 \text{ W} \times 1.2 = \mathbf{200 \text{ W}}$

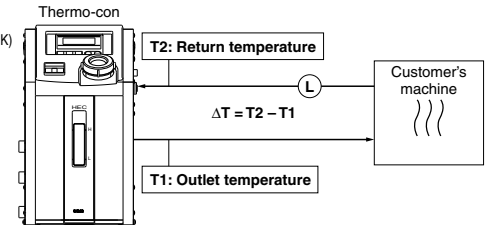

### Example 3 When cooling the object below a certain temperature in certain period of time.

Cooled substance total volume **V** : 20 L  
 Cooling time **h** : 15 min  
 Cooling temperature difference  $\Delta T$  : Temperature difference: 10°C (10 K). Cool from 30°C (303 K) to 20°C (293 K).  
 Circulating fluid : Clear water  
 Density  $\gamma$ :  $1 \times 10^3 \text{ kg/m}^3$   
 Specific heat **C**:  $4.2 \times 10^3 \text{ J/(kg} \cdot \text{K)}$


\* Refer to the information shown below for the typical physical property values by circulating fluid.

$$Q = \frac{\Delta T \times V \times \gamma \times C}{h \times 60 \times 1000}$$

$$= \frac{10 \times 20 \times 1 \times 10^3 \times 4.2 \times 10^3}{15 \times 60 \times 1000}$$

$$= 933 \text{ W}$$

Cooling capacity = Considering a safety factor of 20%,  
 $933 \text{ W} \times 1.2 = \mathbf{1120 \text{ W}}$

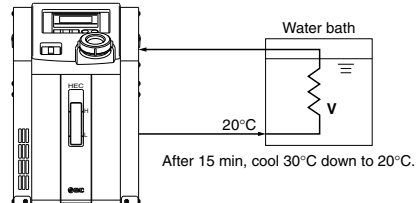

## Precautions on Model Selection

The flow rate of the circulating fluid depends on the pressure loss of the customer's machine and the length, diameter and resistance created by bends in the circulating fluid piping, etc. Check if the required flow rate of circulating fluid can be obtained before selecting.

## Circulating Fluid Typical Physical Property Values

### Fluorinated Fluids

Physical property value	Density $\gamma$ [kg/m <sup>3</sup> ]	Specific heat <b>C</b> [J/(kg · K)]
Temperature		
-10°C	$1.87 \times 10^3$	$0.87 \times 10^3$
20°C	$1.80 \times 10^3$	$0.96 \times 10^3$
50°C	$1.74 \times 10^3$	$1.05 \times 10^3$
80°C	$1.67 \times 10^3$	$1.14 \times 10^3$


### Water

Density  $\gamma$ :  $1 \times 10^3 \text{ [kg/m}^3\text{]}$


Specific heat **C**:  $4.2 \times 10^3 \text{ [J/(kg} \cdot \text{K)]}$



# Peltier-Type Chiller Thermo-con (Air-cooled) Series *HEC-A*



## How to Order

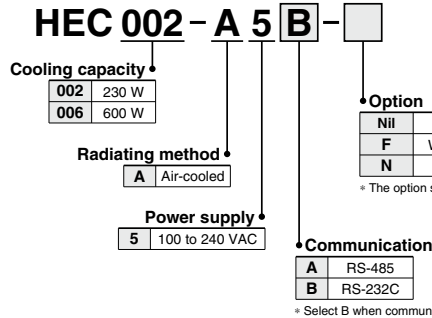

## Specifications (For details, please consult our "Product Specifications" information.)

Model		HEC002-A5A	HEC002-A5B	HEC006-A5A	HEC006-A5B	
Cooling method		Thermoelectric device (Thermo-module)				
Radiating method		Forced air cooling				
Control method		Cooling/Heating automatic shift PID control				
Ambient temperature/humidity		10 to 35°C, 35 to 80%RH (no condensation)				
Circulating fluid system	Circulating fluid		Clear water			
	Operating temperature range		10.0 to 60.0°C (no condensation)			
	Cooling capacity		230 W <small>Note 1)</small>	600 W <small>Note 2)</small>		
	Heating capacity		600 W <small>Note 1)</small>	900 W <small>Note 2)</small>		
	Temperature stability <small>Note 3)</small>		±0.01 to ±0.03°C			
	Pump capacity		Refer to performance chart.			
	Tank capacity		Approx. 1.2 L			
	Port size	IN/OUT	Rc1/4		Rc3/8	
		Drain	Rc1/4 (with plug)			
	Wetted parts material		Stainless steel 303, Stainless steel 304, EPDM, Ceramics, PPS glass 30%, Carbon, PE, Polyurethane			
Electrical system	Power supply		Single-phase 100 to 240 VAC ±10%, 50/60 Hz			
	Overcurrent protector		15 A			
	Current consumption		8 A (100 VAC) to 3 A (240 VAC)	10 A (100 VAC) to 4 A (240 VAC)		
	Alarm		Refer to alarm function.			
	Communications		RS-485	RS-232C	RS-485	RS-232C
	Weight		Approx. 17.5 kg (including foot for fixing)		Approx. 27.5 kg (including foot for fixing)	
	Accessories		Power cable, Foot for fixing			
Safety standards		CE marking, UL (NRTL) standards, Safety standard for medical equipment (IEC 60601-1)		CE marking, UL (NRTL) standards		

Note 1) Conditions: Set temperature 25°C, Ambient temperature 25°C, Circulating flow rate 3 L/min

Note 2) Conditions: Set temperature 25°C, Ambient temperature 20°C, Circulating flow rate 8 L/min

Note 3) The indicated values are with a stable load without turbulence in the operating conditions. It may be out of this range in some other operating conditions.




## Cooling Capacity

The values shown on the performance chart are not guaranteed, but typical. Allow margins for safety when selecting the model.


### HEC002

Circulating fluid: Clear water

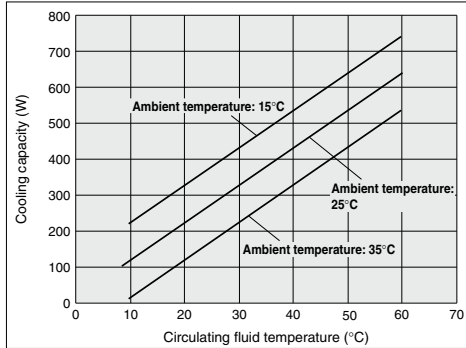

### HEC006


Circulating fluid: Clear water

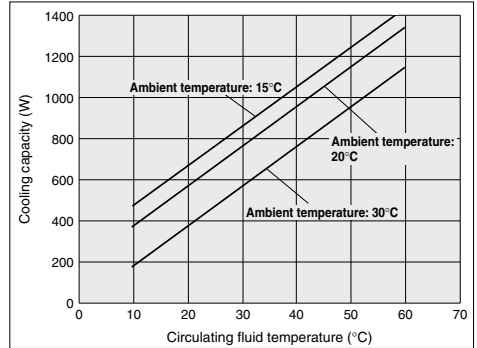

## Heating Capacity


### HEC002

Circulating fluid: Clear water

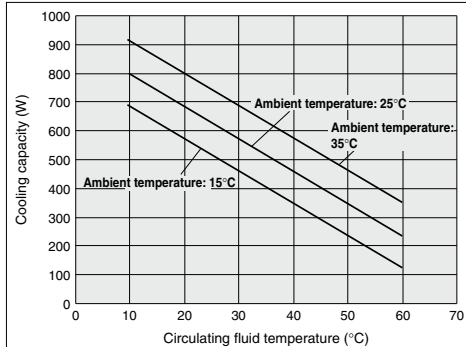

### HEC006

Circulating fluid: Clear water

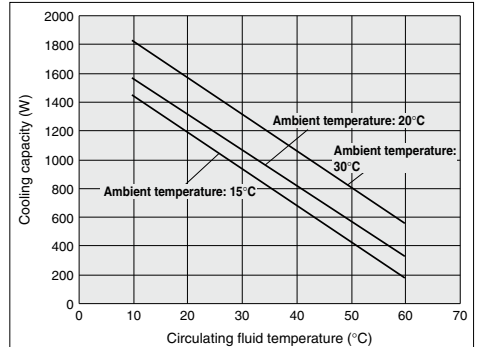


## Pump Capacity (Thermo-con Outlet)

The pressure on the y-axis shows the discharge pressure of circulating fluid in the Thermo-con.


### HEC002

Circulating fluid: Clear water

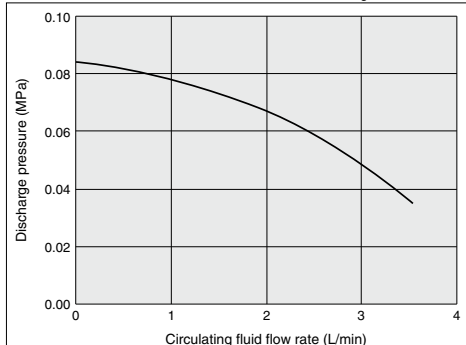

### HEC006

Circulating fluid: Clear water

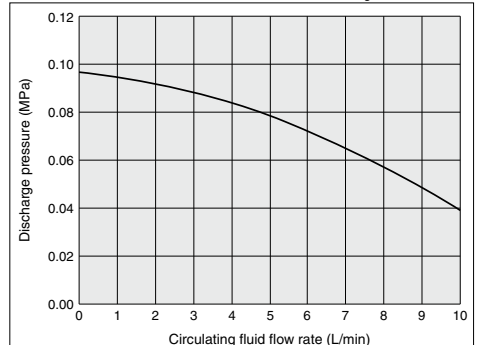

HRG

HRS

HRZ

HRZD

HRW

HEC

HEB



HED

HEA



IDH

**Parts Description**

**HEC002**

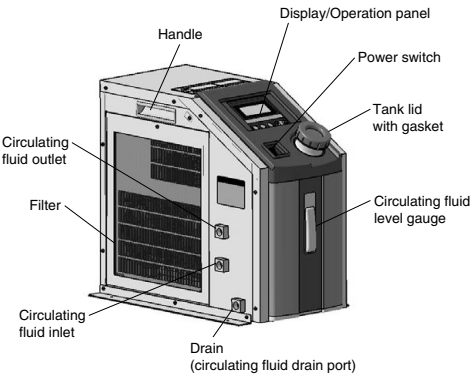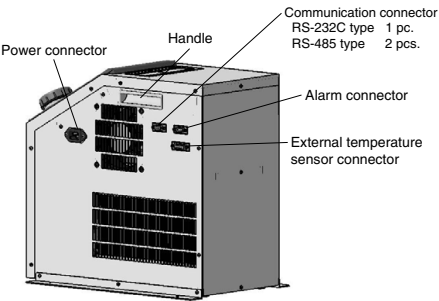


**HEC006**

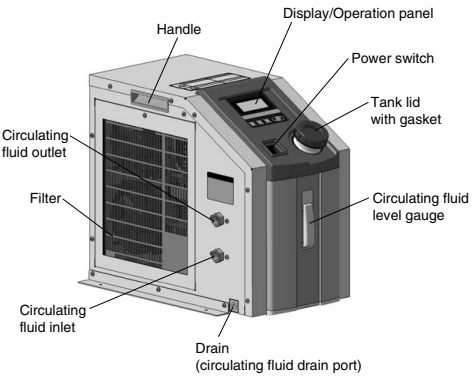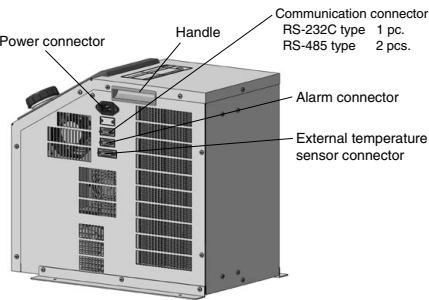


## Dimensions

### HEC002

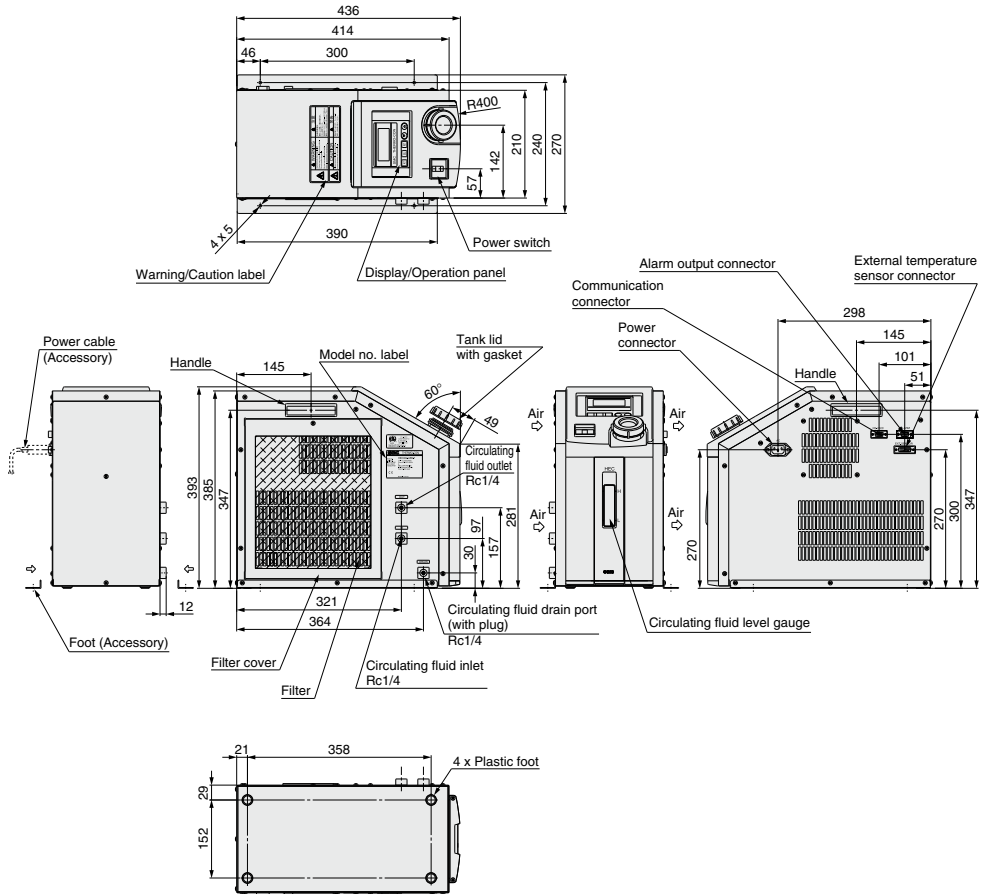

### Option (Fitting part)

NPT fitting specification (-N, -FN)

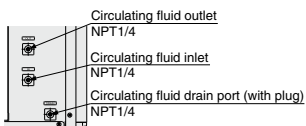

### Power Cable (Accessory)

Connector: IEC 60320 C13 or equivalent  
Cable: 14AWG, O.D. ø8.4

Wire color	Contents
Black	100 to 240 VAC
Black	100 to 240 VAC
Green/Yellow	PE



HRG

HR5

HRZ

HRZD

HRW

**HEC**

HEB

HED

HEA

IDH




## Connectors

### 1. Power connector (AC)

IEC 60320 C14 or equivalent

Pin No.	Contents
1	100 to 240 VAC
2	100 to 240 VAC
3	PE




### 2. Communication connector (RS-232C or RS-485)

D-sub 9 pin (socket)

Holding screw: M2.6

Pin No.	Signal contents	
	RS-232C	RS-485
1	Unused	BUS+
2	RD	BUS-
3	SD	Unused
4	Unused	Unused
5	SG	SG
6-9	Unused	Unused




### 3. External sensor connector (EXT.SENSOR)

D-sub 15 pin (socket)

Holding screw: M2.6

Pin No.	Signal contents
1-2	Unused
3	Terminal A of resistance temperature detector
4	Terminal B of resistance temperature detector
5	Terminal B of resistance temperature detector
6-14	Unused
15	FG




### 4. Alarm output connector (ALARM)

D-sub 9 pin (pin)

Holding screw: M2.6

Pin No.	Signal contents
1	Contact a for output cut-off alarm (open when alarm occurs)
2	Common for output cut-off alarm
3	Contact b for output cut-off alarm (closed when alarm occurs)
4-5	Unused
6	Contact a for upper/lower temp. limit alarm (open when alarm occurs)
7	Common for upper/lower temp. limit alarm
8	Contact b for upper/lower temp. limit alarm (closed when alarm occurs)
9	Unused



HRG

HRS

HRZ

HRZD

HRW

**HEC**

HEB

HED

HEA

IDH

## Alarm

This unit is equipped as standard with a function allowing 15 kinds of alarms to display on the LCD and can be read out by serial communication. Also, it can generate relay output for upper/lower temperature limit alarm and output cut-off alarm.

### Alarm

Alarm code	Alarm description	Operation status	Main reason
WRN	Upper/Lower temp. limit alarm	Continue	The temperature has exceeded the upper or lower limit of the target temperature.
ERR00	CPU hung-up	Stop	The CPU has crashed due to noise, etc.
ERR01	CPU check error	Stop	The contents of the CPU cannot be read out correctly when the power supply is turned on.
ERR03	Back-up data error	Stop	The contents of the back-up data cannot be read out correctly when the power supply is turned on.
ERR04	EEPROM writing error	Stop	The data cannot be written to EEPROM.
ERR11	DC power supply failure	Stop	The DC power supply has failed (due to fan stop or abnormal high temperature) or the thermo-module has been short-circuited.
ERR12	Internal temp. sensor high temp. error	Stop	The internal temperature sensor has exceeded the upper limit of cut-off temperature.
ERR13	Internal temp. sensor low temp. error	Stop	The internal temperature sensor has exceeded the lower limit of cut-off temperature.
ERR14	Thermostat alarm	Stop	The thermostat has been activated due to filter clog or fan/pump failure, etc.
ERR15	Abnormal output alarm	Continue	The temperature cannot be changed even at 100% output due to overload or disconnection of the thermo-module.
ERR16	Low flow rate alarm (option)	Stop	The flow rate of the circulating fluid has dropped.
ERR17	Internal temp. sensor disconnection alarm	Stop	The internal temperature sensor has been disconnected or short-circuited.
ERR18	External temp. sensor disconnection alarm	Continue	The external temperature sensor has been disconnected or short-circuited. (Only detected when in learning control or external tune control)
ERR19	Abnormal auto tuning alarm	Stop	Auto tuning has not been completed within 20 minutes.
ERR20	Low fluid level alarm	Stop	The amount of circulating fluid in the tank has dropped.

## Maintenance

Maintenance of this unit is performed only in the form of return to and repair at SMC's site. As a rule, SMC will not conduct on-site maintenance. Separately, the following parts have a limited life and need to be replaced before the life ends.

### Parts Life Expectation

Description	Expected life	Possible failure
Pump	3 to 5 years	The bearing is worn so the pump fails to transfer the circulating fluid, which results in temperature control failure.
Fan	5 to 10 years	The bearing uses up lubrication and makes the fan unable to supply enough air, which deteriorates the cooling and heating capacity.
DC power supply	5 to 10 years	The capacity of the electrolytic condenser decreases, and causes abnormal voltage which results in DC power supply failure and stops the Thermo-con.
Display panel	50,000 hours (approx. 5 years)	The display turns off when the backlight of the LCD reaches the end of its life.

# Series HEC-A

## Options

Note) Options have to be selected when ordering the Thermo-con. It is not possible to add them after purchasing the unit.

### F Option symbol

#### With Flow Switch

HEC  -    - F

• With flow switch

This is an ON/OFF switch detecting low levels of the circulating fluid.  
When the fluid volume is 1 L/min. or less, "ERR16" is displayed and the Thermo-con stops. This switch is installed between the circulating fluid inlet and the tank, and built into the Thermo-con. Refer to page 1381.

Type	Applicable model
Air-cooled	HEC002-A5□-F HEC006-A5□-F

### N Option symbol

#### NPT Thread

HEC  -    - N

• NPT thread

The connection parts of circulating fluid piping, facility water piping and circulating fluid drain port are NPT thread type.

Type	Applicable model
Air-cooled	HEC002-A5□-N HEC006-A5□-N

HRG

HRS

HRZ

HRZD

HRW

**HEC**

HEB

HED

HEA

IDH





## Series HEC-A

# Specific Product Precautions 1

Be sure to read this before handling. Refer to front matter 41 for Safety Instructions and pages 1246 to 1249 for Temperature Control Equipment Precautions.

### System Design

#### ⚠ Warning

##### 1. This catalog shows the specifications of the Thermo-con.

1. Check detailed specifications in the separate "Product Specifications", and evaluate the compatibility of the Thermo-con with customer's system.
2. Although the protection circuit as a single unit is installed, the customer is requested to carry out the safety design for the whole system.

### Handling

#### ⚠ Warning

##### 1. Thoroughly read the Operation Manual.

Read the Operation Manual completely before operation, and keep this manual available whenever necessary.

##### 2. If the set temperature is repeatedly changed by 10°C or more, the Thermo-con may fail in short periods of time.

### Operating Environment/Storage Environment

#### ⚠ Warning

##### 1. Keep within the specified ambient temperature and humidity range.

Also, if the set temperature is too low, condensation may form on the inside of the Thermo-con or the surface of piping even within the specified ambient temperature range. Dew condensation can cause failure, and so must be avoided by considering operating conditions.

##### 2. The Thermo-con is not designed for clean room usage.

It generates dust from the pump inside the unit and the cooling fan.

##### 3. Low molecular siloxane can damage the contact of the relay.

Use the Thermo-con in a place free from low molecular siloxane.

### Radiation Air



#### ⚠ Caution

##### 1. The inlet for radiation air must not be exposed to particles and dust as far as possible.



##### 2. Do not let the inlet and outlet for radiation air get closed.

###### <HEC002>

If radiation is prevented, the set temperature may not be achieved depending on the value of the set temperature and the load. Keep a space of 100 mm for opened rear side or 200 mm for closed rear side respectively.

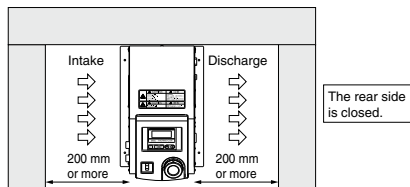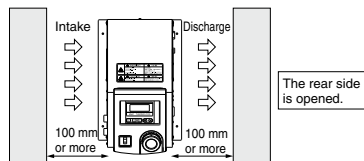

###### <HEC006>

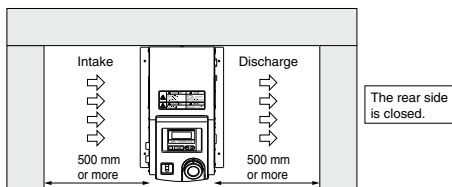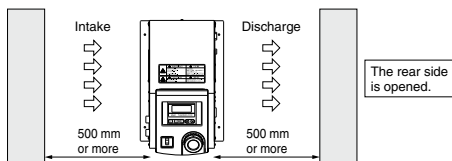

Note) The space must be 500 mm or more. Be sure that the ambient temperature is within the specification range.



## Series HEC-A

# Specific Product Precautions 2

Be sure to read this before handling. Refer to front matter 41 for Safety Instructions and pages 1246 to 1249 for Temperature Control Equipment Precautions.

### Radiation Air

#### ⚠ Caution

- If more than one Thermo-con is used, consider their arrangement so that the downstream sides of the Thermo-cons suck radiation air from the upstream sides.

Otherwise, the performance at the downstream sides may deteriorate. Also, the set temperature may not be achieved depending on the value of the set temperature and the load. In such a case, take countermeasures such as changing the direction of the Thermo-cons to prevent the deterioration of performance.

- If dust adheres to the filter, remove dust with a vacuum cleaner or a dry cloth.
- Do not operate without the filter.  
Otherwise, dust may accumulate on the heat sink and electrical components, causing abnormal heating.

### Circulating Fluid

#### ⚠ Caution

- Use tap water or fluid which will not damage the wetted material.  
(Stainless steel 303, Stainless steel 304, EPDM, Polypropylene, PE, PPE, Ceramics, Polyurethane)

- Deionized water (with an electrical conductivity of approx. 1  $\mu\text{S}/\text{cm}$ ) can be used, but may lose its electrical conductivity.

Also, if a facility supplying deionized water is used, the Thermo-con may be damaged by static electricity.

- If deionized water is used, bacteria and algae may grow in short periods of time.

If the Thermo-con is operated with bacteria and algae, its cooling capacity or the capacity of the pump may deteriorate. Exchange all deionized water regularly depending on the conditions (once a month as a guide).

- If using a fluid other than water, please contact SMC beforehand.

- The maximum operating pressure of circulating fluid circuit is 0.1 MPa.

If this pressure is exceeded, leakage from the tank in the Thermo-con can result.

- Select a pipe with a length and diameter which allow a flow rate of 1 L/min or more (HEC002) or 3 L/min or more (HEC006) for the circulating fluid.

If the flow rate is less than these values, the Thermo-con cannot provide precise control, but also can fail because of the repeated cooling and heating operation.

- A magnet driven pump is used as a circulating pump.

A fluid which contains metal powders such as iron powder cannot be used.

- The Thermo-con must not be operated without circulating fluid.

The pump can break due to idling.

### Circulating Fluid

#### ⚠ Caution

- If the tank lid is opened after the supply of circulating fluid, the circulating fluid may spill out depending on the condition of external piping.

- If an external tank is used, the circulating fluid may spill out from the internal tank lid depending on where the external tank is installed.

Check that the internal tank has no leakage if using an external tank.

- If there is a point where fluid is released to atmosphere externally (tank or piping), minimize the piping resistance at the circulating fluid return side.

If the piping resistance is too large, the piping may be crushed, or the built-in circulator tank may be deformed or cracked because the pressure in the piping for return will become negative. The built-in circulator tank is made of resin (PE). Therefore, the tank may be crushed if the pressure is negative. Special attention must be paid if the flow rate of the circulating fluid is high. To avoid getting negative pressure less than  $-0.02$  MPa, the piping for return should be as thick and short as possible to minimize the piping resistance. It is also effective to restrict the flow rate of circulating fluid or remove the gasket of internal tank for the release to atmosphere.

- Fluorinated fluid is outside of the specifications.

If it is used in the Thermo-con, static electricity will be generated by the flow of fluid. This static electricity may be discharged to the board of the Thermo-con, causing damage or operation failure and loss of data of such as set temperature. Also, as the specific gravity of the fluorinated fluid is 1.5 to 1.8 times of water, the pump will be overloaded, which also causes fluorinated fluid to be outside the specifications. Therefore, if fluorinated fluid is used, please contact SMC and we will introduce a suitable special product (water-cooled type).

- Avoid operation with cavitation or bubbles due to low fluid level in the tank. This may shorten the pump life.

- If clear water is used, it should satisfy the quality standards shown below.

#### Clear Water (as Circulating Water) Quality Standards

The Japan Refrigeration and Air Conditioning Industry Association

JRA GL-02-1994 "Cooling water system - Circulating type - Supply water"

	Item	Unit	Standard value	Influence	
				Corrosion	Scale generation
Standard item	pH (at 25°C)	—	6.0 to 8.0	○	○
	Electrical conductivity (25°C)	[ $\mu\text{S}/\text{cm}$ ]	100* to 300*	○	○
	Chloride ion ( $\text{Cl}^-$ )	[mg/L]	50 or less	○	
	Sulfuric acid ion ( $\text{SO}_4^{2-}$ )	[mg/L]	50 or less	○	
	Acid consumption amount (at pH4.8)	[mg/L]	50 or less		○
	Total hardness	[mg/L]	70 or less		○
	Calcium hardness ( $\text{CaCO}_3$ )	[mg/L]	50 or less		○
	Ionic state silica ( $\text{SiO}_2$ )	[mg/L]	30 or less		○
Reference item	Iron (Fe)	[mg/L]	0.3 or less	○	○
	Copper (Cu)	[mg/L]	0.1 or less	○	
	Sulfide ion ( $\text{S}_2^{2-}$ )	[mg/L]	Should not be detected.	○	
	Ammonium ion ( $\text{NH}_4^+$ )	[mg/L]	0.1 or less	○	
	Residual chlorine (Cl)	[mg/L]	0.3 or less	○	
	Free carbon ( $\text{CO}_2$ )	[mg/L]	4.0 or less	○	

\* In the case of [ $\text{M}\Omega \cdot \text{cm}$ ], it will be 0.003 to 0.01.

○: Factors that have an effect on corrosion or scale generation.

• Even if the water quality standards are met, complete prevention of corrosion is not guaranteed.



## Series *HEC-A*

# Specific Product Precautions 3

Be sure to read this before handling. Refer to front matter 41 for Safety Instructions and pages 1246 to 1249 for Temperature Control Equipment Precautions.

### Communication

#### **Caution**

**1. The set value can be written to EEPROM, but only up to approx. 1 million times.**

In particular, pay attention to how many of times the writing is performed using the communication function.

### Maintenance

#### **Warning**

**1. Prevention of electric shock and fire**

Do not operate the switch with wet hands. Also, do not operate the Thermo-con with water left on it.

**2. Action in the case of error**

If any error such as abnormal sounds, smoke, or bad smell occurs, cut off the power at once, and stop supplying and conveying fluid. Please contact SMC or a sales distributor to repair the Thermo-con.

**3. Regular inspection**

Check the following items at least once a month. The inspection must be done by an operator who has sufficient knowledge and experience.

- a) Check of displayed contents.
- b) Check of temperature, vibration and abnormal sounds in the body of the Thermo-con.
- c) Check of the voltage and current of the power supply system.
- d) Check for leakage and contamination of the circulating fluid and intrusion of foreign objects to it, and subsequent replacement of the fluid.
- e) Check for flow condition, temperature and filter of radiation air.

HRG
HRS
HRZ
HRZD
HRW
<b>HEC</b>
HEB
HED
HEA
IDH

# Peltier-Type Chiller Thermo-con (Water-cooled) Series **HEC-W**



Note) Except  
HEC006, 012



## How to Order

140 W, 320 W

**HEC** **003** - **W** **5** **B** -

Cooling capacity

001	140 W
003	320 W

Radiating method

W	Water-cooled
---	--------------

Power supply

5	100 to 240 VAC
---	----------------

Option

Nil	None
F	With flow switch
N	NPT thread
L	With level switch

\* The option should be  
specified when ordering.

Communication

A	RS-485
B	RS-232C

\* Select B when  
communication is not used.



## Specifications (For details, please consult our "Product Specifications" information.)

Model	HEC001-W5A	HEC001-W5B	HEC003-W5A	HEC003-W5B
Cooling method	Thermoelectric device (Thermo-module)			
Radiating method	Water-cooled			
Control method	Cooling/Heating automatic shift PID control			
Ambient temperature/humidity	10 to 35°C, 35 to 80%RH (no condensation)			
Circulating fluid system	Circulating fluid	Clear water, 20% ethylene glycol		
	Operating temp. range	10.0 to 60.0°C (no condensation)		
	Cooling capacity	140 W <small>Note 1)</small>		320 W <small>Note 1)</small>
	Heating capacity	400 W <small>Note 1)</small>		770 W <small>Note 1)</small>
	Temperature stability <small>Note 2)</small>	±0.01 to 0.03°C		
	Pump capacity	Refer to performance chart.		
	Tank capacity	Approx. 1.2 L		
	Port size	IN/OUT: Rc3/8 Drain: Rc1/4 (with plug)		
	Wetted parts material	PPE, PP glass 10%, Alumina ceramics, Carbon, EPDM, Stainless steel 303, Stainless steel 304, PE, PP, NBR		
	Temperature range	10 to 35°C (no condensation)		
Facility water system	Pressure range	Within 1 MPa		
	Required flow rate <small>Note 3)</small>	3 to 7 L/min		
	Port size	IN/OUT: Rc3/8		
	Wetted parts material	Stainless steel 304		
Electrical system	Power supply	Single-phase 100 to 240 VAC ±10%, 50/60 Hz		
	Overcurrent protector	10 A		
	Current consumption	3.5 A (100 VAC) to 1.5 A (240 VAC)		5.5 A (100 VAC) to 2.5 A (240 VAC)
	Alarm	Refer to alarm function.		
	Communications	RS-485	RS-232C	RS-485 RS-232C
	Weight	Approx. 12 kg		Approx. 13 kg
	Accessories	Power cable, Foot for fixing, Splashproof cover		
	Safety standards	CE marking, UL (NRTL) standards, SEMI		

Note 1) Circulating fluid/Clear water conditions: Circulating fluid set temperature 20°C, Flow rate 5 L/min., Facility water temperature 20°C, Flow rate 5 L/min., Ambient temperature 25°C  
Note 2) The indicated values are with a stable load without turbulence in the operating conditions. It may be out of this range in some other operating conditions.  
Note 3) The flow rate over or below the set range may deteriorate performance or generate noise.

# Peltier-Type Chiller Thermo-con (Water-cooled) **Series HEC-W**

## How to Order

600 W, 1200 W

**HEC 012 - W 2 B -**

Cooling capacity

006	600 W
012	1200 W

Radiating method

W	Water-cooled
---	--------------

Power supply

2	200 to 220 VAC
---	----------------

Option

Nil	None
N	NPT thread

\* The option should be specified when ordering.

Communication

A	RS-485
B	RS-232C

\* Select B when communication is not used.



## Specifications (For details, please consult our "Product Specifications" information.)

Model		HEC006-W2A	HEC006-W2B	HEC012-W2A	HEC012-W2B
Cooling method		Thermoelectric device (Thermo-module)			
Radiating method		Water-cooled			
Control method		Cooling/Heating automatic shift PID control			
Ambient temperature/humidity		10 to 35°C, 35 to 80%RH (no condensation)			
Circulating fluid system	Circulating fluid <sup>Note 1)</sup>	Clear water, Fluorinated fluid (Fluorinert™ FC-3283, GALDEN® HT135)			
	Operating temperature range	10.0 to 60.0°C (no condensation)			
	Cooling capacity	600 W (Clear water), 400 W (Fluorinert™ FC-3283) <sup>Note 2)</sup>	1200 W (Clear water), 800 W (Fluorinert™ FC-3283) <sup>Note 3)</sup>		
	Heating capacity	900 W (Clear water), 600 W (Fluorinert™ FC-3283) <sup>Note 2)</sup>	2200 W (Clear water), 1500 W (Fluorinert™ FC-3283) <sup>Note 3)</sup>		
	Temperature stability <sup>Note 4)</sup>	±0.01 to 0.03°C			
	Pump capacity	Refer to performance chart.			
	Tank capacity	Approx. 3 L		Approx. 5 L	
Facility water system	Port size	IN/OUT: Rc3/8 Drain: Rc1/4 (with plug)		IN/OUT: Rc3/4 Drain: Rc1/4 (with plug)	
	Wetted parts material	Stainless steel 303, Stainless steel 304, EPDM, Ceramics, PPS glass 30%, Carbon, PE, Polyurethane		Stainless steel 303, Stainless steel 304, EPDM, Ceramics, PP, PE, Polyurethane, SiC, PPS	
	Temperature range	10 to 35°C (no condensation)			
Electrical system	Pressure range	Within 1 MPa			
	Required flow rate <sup>Note 5)</sup>	8 to 10 L/min		10 to 15 L/min	
	Port size	IN/OUT: Rc3/8		IN/OUT: Rc1/2	
Electrical system	Wetted parts material	Stainless steel 303, Stainless steel 304			
	Power supply	Single-phase 200 to 220 VAC ±10%, 50/60 Hz			
	Overcurrent protector	10 A		15 A	
	Current consumption	5 A		10 A	
	Alarm	Refer to alarm function.			
	Communications	RS-485	RS-232C	RS-485	RS-232C
	Weight	Approx. 25 kg (including foot for fixing)		Approx. 40 kg (including foot for fixing)	
Accessories		Power cable, Foot for fixing			
Safety standards		CE marking			

Note 1) Fluorinert™ is a trademark of 3M and GALDEN® is a registered trademark of Solvay Solexis, Inc. Regarding the fluid other than the above, please consult with SMC.

Note 2) Conditions: Set temperature 25°C, Facility water temperature 20°C, Facility water flow rate 8 L/min, Ambient temperature 25°C.

Note 3) Conditions: Set temperature 25°C, Facility water temperature 20°C, Facility water flow rate 10 L/min, Ambient temperature 25°C.

Note 4) The indicated values are with a stable load without turbulence in the operating conditions. It may be out of this range in some other operating conditions.

Note 5) The flow rate over or below the set range may deteriorate performance or generate noise.


# Series HEC-W

## Cooling Capacity


The values shown on the performance chart are not guaranteed, but typical. Allow margins for safety when selecting the model.

### HEC001

Circulating fluid: Clear water

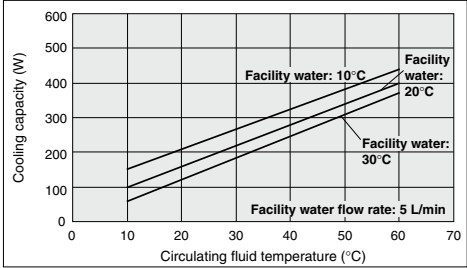


Circulating fluid: 20% ethylene glycol

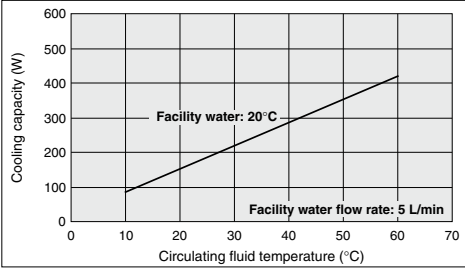


### HEC003

Circulating fluid: Clear water

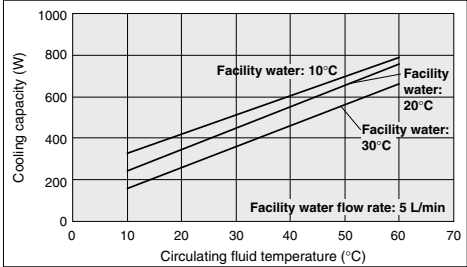


Circulating fluid: 20% ethylene glycol

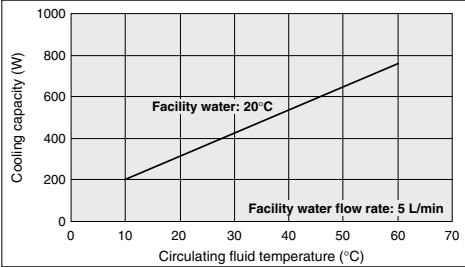


### HEC006

Circulating fluid: Clear water

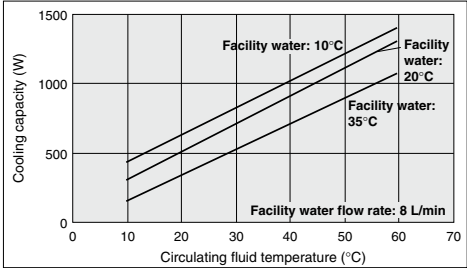


Circulating fluid: FC-3283

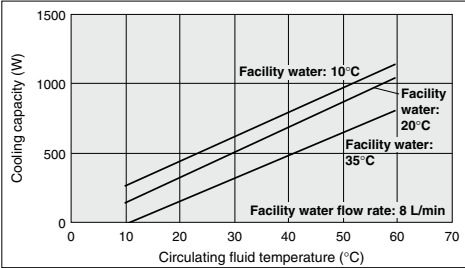


### HEC012

Circulating fluid: Clear water

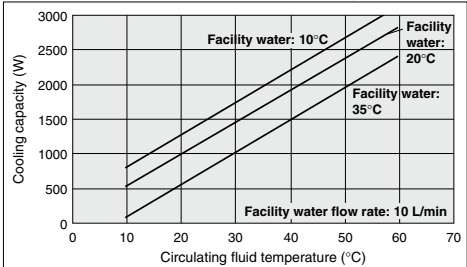

Circulating fluid: FC-3283

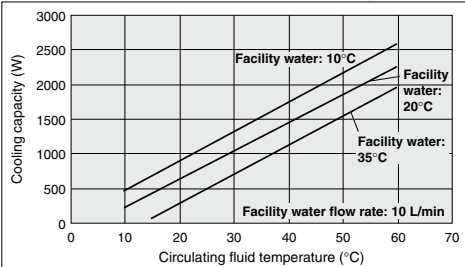




## Heating Capacity


The values shown on the performance chart are not guaranteed, but typical. Allow margins for safety when selecting the model.

### HEC001

Circulating fluid: Clear water

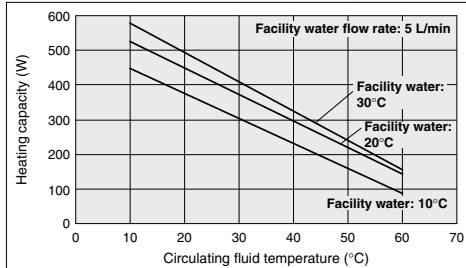


Circulating fluid: 20% ethylene glycol

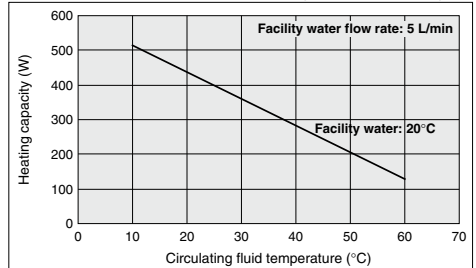


### HEC003

Circulating fluid: Clear water

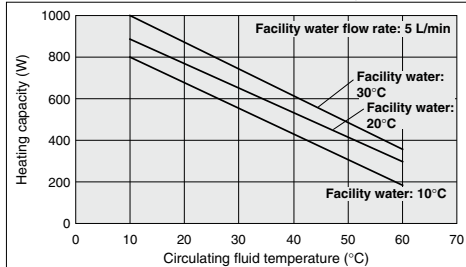


Circulating fluid: 20% ethylene glycol

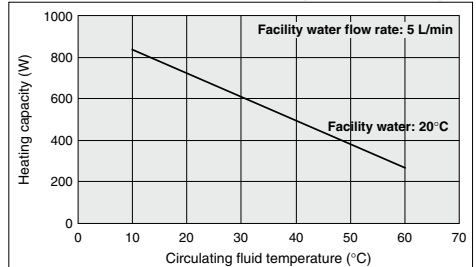


### HEC006

Circulating fluid: Clear water

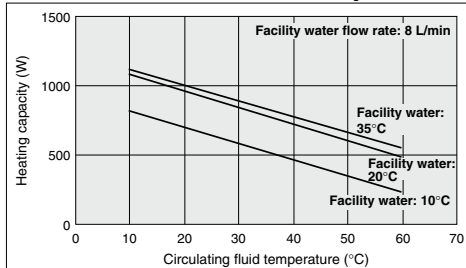


Circulating fluid: FC-3283

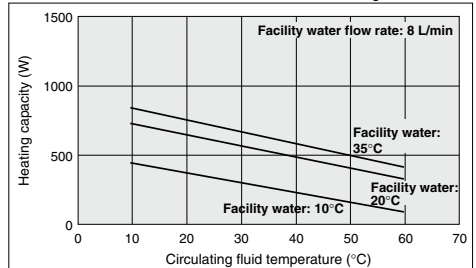


### HEC012

Circulating fluid: Clear water

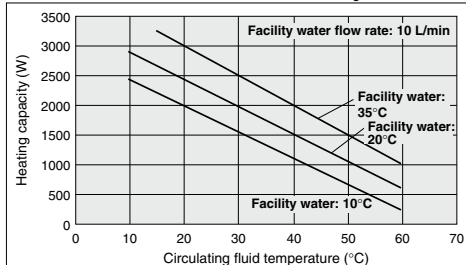

Circulating fluid: FC-3283

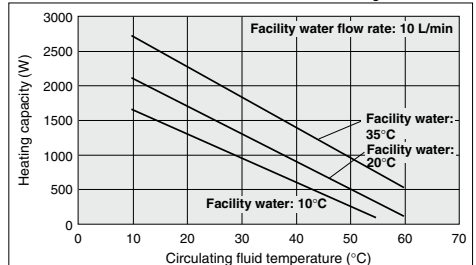

HRG

HRs

HRZ

HRZD

HRW

**HEC**

HEB


HED

HEA


IDH

**Pump Capacity (Thermo-con Outlet)**


**HEC001/003** Since a DC pump is used, the unit is not affected by power requirements.

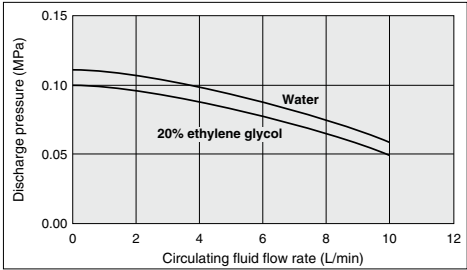

**HEC006** Since a DC pump is used, the unit is not affected by power requirements.

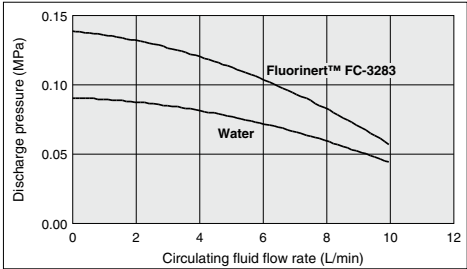


**HEC012**

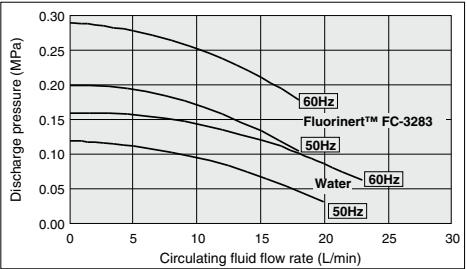


**Pressure Loss in Facility Water Circuit**


**HEC001**

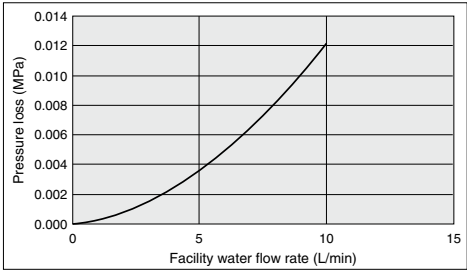


**HEC003**

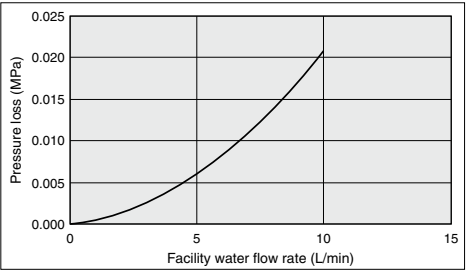

**HEC006**

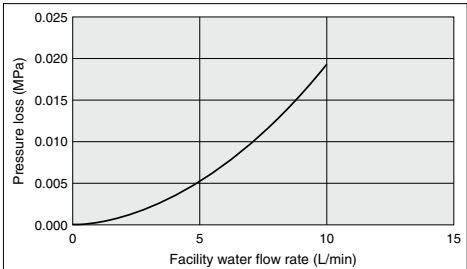


**HEC012**

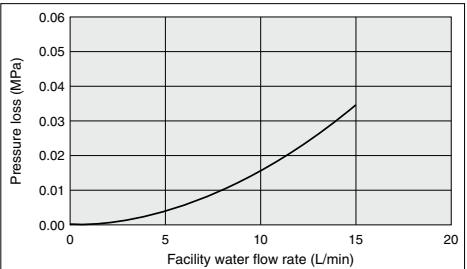


Parts Description

HEC001/003

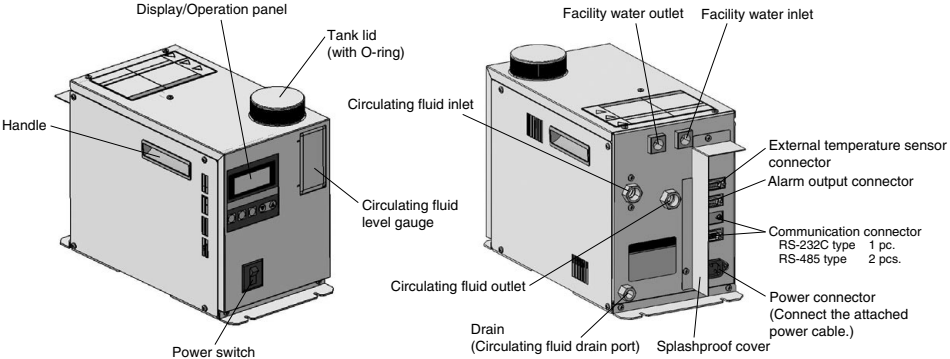

HEC006/012

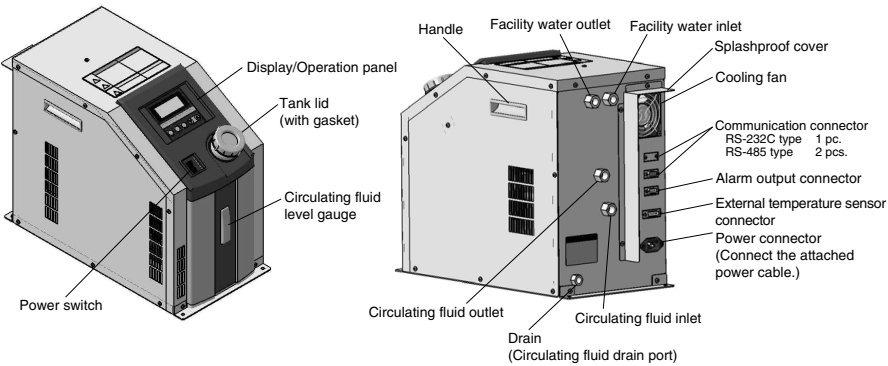


HRG
HRS
HRZ
HRZD
HRW
<b>HEC</b>
HEB
HED
HEA
IDH

# Series HEC-W

## Dimensions

HEC001-W5□

HEC003-W5□

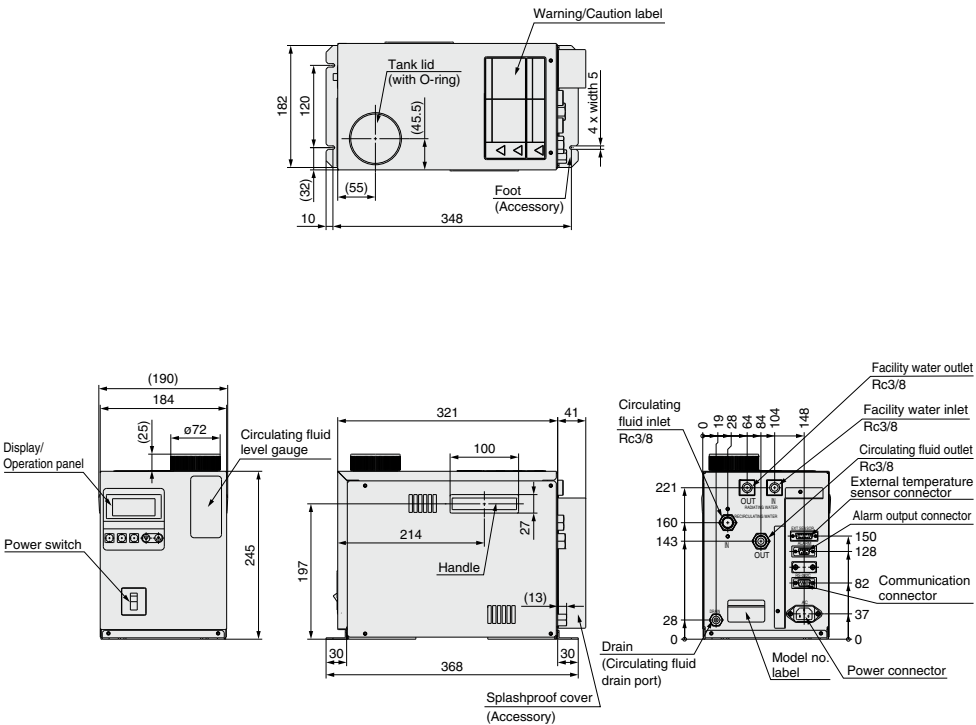


For NPT thread specification (-N), all fittings (including those at the circulating fluid drain port) are made of NPT.

## Power Cable (Accessory)




Connector: IEC 60320 C13 or equivalent  
Cable: 14AWG, O.D. ø8.4

Wire color	Contents
Black	100 to 240 VAC
Black	100 to 240 VAC
Green/Yellow	PE



Power cable (Accessory)

## Dimensions

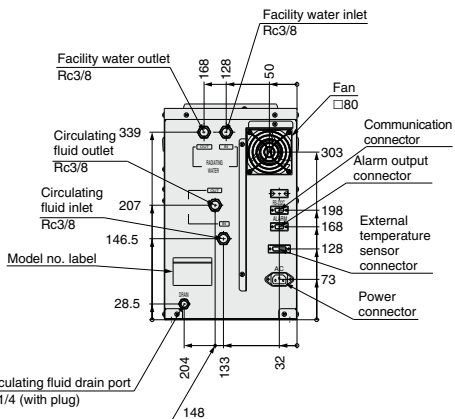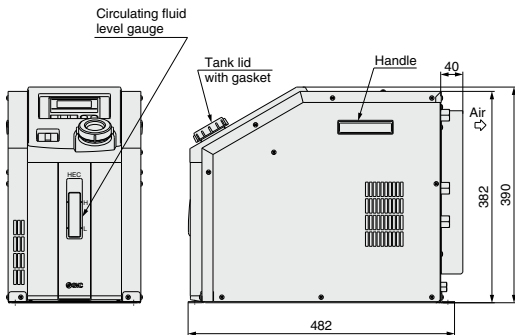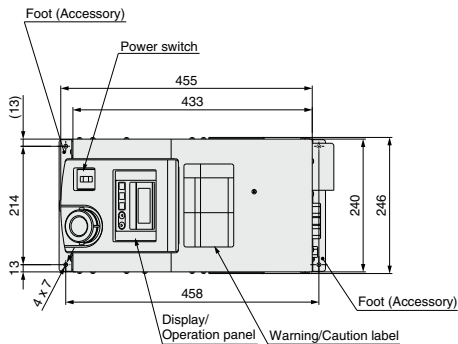
HEC006-W2 ☐

For NPT thread specification (-N), all fittings (including those at the circulating fluid drain port) are made of NPT.

## Power Cable

Connector: IEC 60320 C13 or equivalent  
Cable: 14AWG, O.D. ø8.4

Wire color	Contents
Black	200 to 220 VAC
Black	200 to 220 VAC
Green/Yellow	PE




**Power cable (Accessory)**

# Series HEC-W

## Dimensions

HEC012-W2□

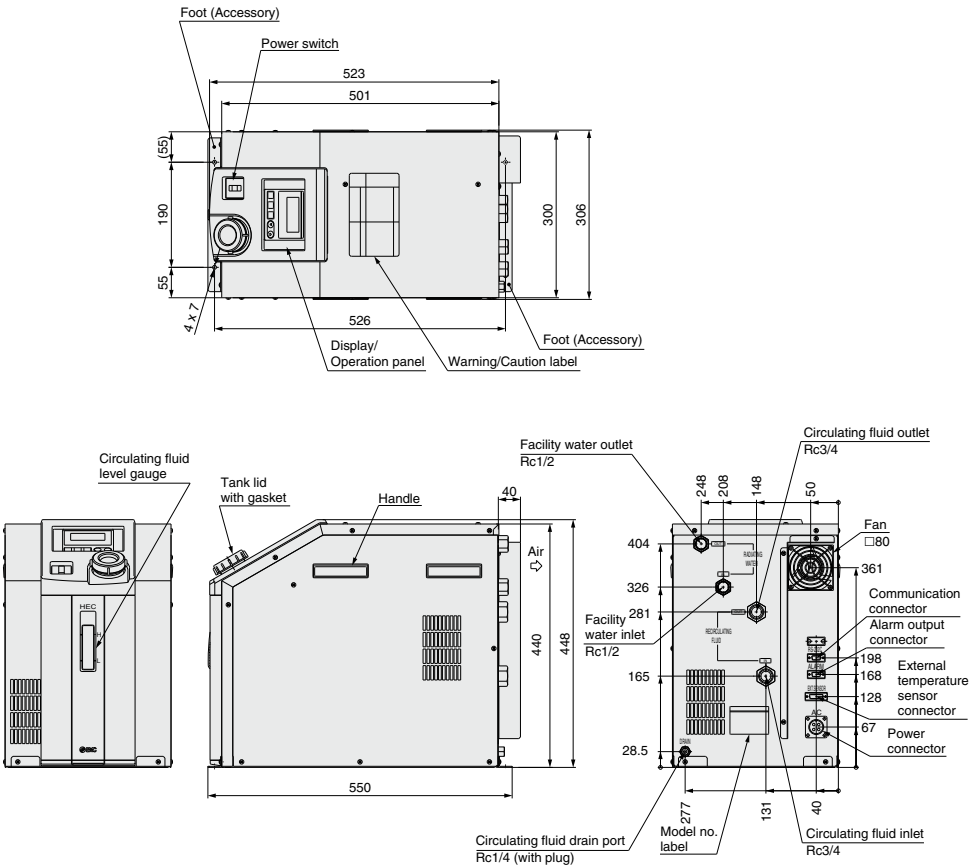


For NPT fitting specification (-N), all fittings (including those at the circulating fluid drain port) are made of NPT.

## Power Cable

Connector: DDK CE05-6A18-10SD-D-BSS or equivalent  
Cable: 14AWG, O.D. ø8.4

Wire color	Contents
Black	200 to 220 VAC
Black	200 to 220 VAC
Green/Yellow	PE



Power cable (Accessory)

## Connectors

### HEC006-W2□/001-W5□/003-W5□

#### 1. Power connector (AC)

IEC 60320 C14 or equivalent


HEC006-W2□

Pin No.	Contents
1	200 to 220 VAC
2	200 to 220 VAC
3	PE

HEC001-W5□

HEC003-W5□

Pin No.	Contents
1	100 to 240 VAC
2	100 to 240 VAC
3	PE




#### 2. Communication connector (RS-232C or RS-485)

D-sub 9 pin (socket)

Holding screw: M2.6

Pin No.	Signal contents	
	RS-232C	RS-485
1	Unused	BUS+
2	RD	BUS-
3	SD	Unused
4	Unused	Unused
5	SG	SG
6-9	Unused	Unused




#### 3. External sensor connector (EXT.SENSOR)

D-sub 15 pin (socket)

Holding screw: M2.6

Pin No.	Signal contents
1-2	Unused
3	Terminal A of resistance temperature detector
4	Terminal B of resistance temperature detector
5	Terminal B of resistance temperature detector
6-14	Unused
15	FG




#### 4. Alarm output connector (ALARM)

D-sub 9 pin (pin)

Holding screw: M2.6

Pin No.	Signal contents
1	Contact a for output cut-off alarm (open when alarm occurs)
2	Common for output cut-off alarm
3	Contact b for output cut-off alarm (closed when alarm occurs)
4-5	Unused
6	Contact a for upper/lower temp. limit alarm (open when alarm occurs)
7	Common for upper/lower temp. limit alarm
8	Contact b for upper/lower temp. limit alarm (closed when alarm occurs)
9	Unused




### HEC012-W2□

#### Power connector (AC)

DDK CE05-2A18-10PD-D or equivalent

Pin No.	Contents
A	200 to 220 VAC
B	200 to 220 VAC
C	Unused
D	PE



Other connectors are the same as those for the HEC006-W2□.



## Alarm

This unit is equipped as standard with a function allowing 15 kinds of alarms to display on the LCD and can be read out by serial communication. Also, it can generate relay output for upper/lower temperature limit alarm and output cut-off alarm.

Alarm code	Alarm description	Operation status	Main reason
WRN	Upper/Lower temp. limit alarm	Continue	The temperature has exceeded the upper or lower limit of the target temperature.
ERR00	CPU hung-up	Stop	The CPU has crashed due to noise, etc.
ERR01	CPU check error	Stop	The contents of the CPU cannot be read out correctly when the power supply is turned on.
ERR03	Back-up data error	Stop	The contents of the back-up data cannot be read out correctly when the power supply is turned on.
ERR04	EEPROM writing error	Stop	The data cannot be written to EEPROM.
ERR11	DC power supply failure	Stop	The DC power supply has failed (due to abnormal high temperature) or an irregular voltage has occurred or the thermo-module has been short-circuited.
ERR12	Internal temp. sensor high temp. error	Stop	The internal temperature sensor has exceeded the upper limit of cut-off temperature.
ERR13	Internal temp. sensor low temp. error	Stop	The internal temperature sensor has exceeded the lower limit of cut-off temperature.
ERR14	Thermostat alarm	Stop	The thermostat has been activated due to insufficient of the facility water or high temperature.
ERR15	Abnormal output alarm	Continue	The temperature cannot be changed even at 100% output due to overload or disconnection of the thermo-module.
ERR16	Pump failure *1 or low circulating fluid level alarm *2	Stop	The pump has been overloaded *1 or the flow switch is activated *2.
ERR17	Internal temp. sensor disconnection alarm	Stop	The internal temperature sensor has been disconnected or short-circuited.
ERR18	External temp. sensor disconnection alarm	Continue	The external temperature sensor has been disconnected or short-circuited. (Only detected when in learning control or external tune control.)
ERR19	Abnormal auto tuning alarm	Stop	Auto tuning has not been completed within 20 minutes.
ERR20	Low fluid level alarm *3	Stop	The amount of circulating fluid in the tank has dropped and the level switch is activated.

\*1 The HEC012 only

\*2 Optional for the HEC001 and HEC003 only (Not available for the HEC006)

\*3 Optional for the HEC001 and HEC003

## Maintenance

Maintenance of this unit is performed only in the form of return to and repair at SMC's site. As a rule, SMC will not conduct on-site maintenance. Separately, the following parts have a limited life and need to be replaced before the life ends.

### Parts Life Expectation

Description	Expected life	Possible failure
Pump	3 to 5 years	The bearing is worn so the pump fails to transfer the circulating fluid, which results in temperature control failure.
Fan	5 to 10 years	The bearing uses up lubrication and makes the fan unable to supply enough air, which increases the internal temperature of the Thermo-con, and activates the overheat protection of the power supply and generates the alarm.
DC power supply	5 to 10 years	The capacity of the electrolytic condenser decreases, and causes abnormal voltage which results in DC power supply failure and stops the Thermo-con.
Display panel	50,000 hours (approx. 5 years)	The display turns off when the backlight of the LCD reaches the end of its life.

# Series HEC-W

## Options

Note) Options have to be selected when ordering the Thermo-con. It is not possible to add them after purchasing the unit.

### **F** Option symbol With Flow Switch

HEC  -    - **F**

• With flow switch

This is an ON/OFF switch detecting low levels of the circulating fluid.  
When the fluid volume is 1 L/min. or less, "ERR16" is displayed and the Thermo-con stops. This switch is installed between the circulating fluid inlet and the tank, and built into the Thermo-con. Refer to page 1381.

Type	Applicable model
Water-cooled	HEC001-W5□-F
	HEC003-W5□-F

### **N** Option symbol NPT Thread

HEC  -    - **N**

• NPT thread

The connection parts of circulating fluid piping, facility water piping and circulating fluid drain port are NPT thread type.

Type	Applicable model
Water-cooled	HEC001-W5□-N
	HEC003-W5□-N
	HEC006-W2□-N
	HEC012-W2□-N

### **L** Option symbol With Level Switch

HEC  -    - **L**

• With level switch

This switch is used to detect a LOW level of tank fluid. When the fluid level becomes below the LOW level, "ERR20" is displayed and the Thermo-con stops. This switch is installed in the circulating fluid tank and built into the Thermo-con. Refer to page 1381.

Type	Applicable model
Water-cooled	HEC001-W5□-L
	HEC003-W5□-L

Other models include a level switch as standard equipment.

HRG

HRS

HRZ

HRZD

HRW

**HEC**

HEB

HED

HEA

IDH



## Series HEC-W

# Specific Product Precautions 1

Be sure to read this before handling. Refer to front matter 41 for Safety Instructions and pages 1246 to 1249 for Temperature Control Equipment Precautions.

### System Design

#### ⚠ Warning

##### 1. This catalog shows the specifications of the Thermo-con.

1. Check detailed specifications in the separate "Product Specifications", and evaluate the compatibility of the Thermo-con with customer's system.
2. Although the protection circuit as a single unit is installed, the customer is requested to carry out the safety design for the whole system.

### Handling

#### ⚠ Warning

##### 1. Thoroughly read the Operation Manual.

Read the Operation Manual completely before operation, and keep this manual available whenever necessary.

##### 2. If the set temperature is repeatedly changed by 10°C or more, the Thermo-con may fail in short periods of time.

### Operating Environment/Storage Environment

#### ⚠ Warning

##### 1. Keep within the specified ambient temperature and humidity range.

Also, if the set temperature is too low, condensation may form on the inside of the Thermo-con or the surface of piping even within the specified ambient temperature range. Dew condensation can cause failure, and so must be avoided by considering operating conditions.

##### 2. The Thermo-con is not designed for clean room usage.

The pump and fan generate dust.

##### 3. Low molecular siloxane can damage the contact of the relay.

Use the Thermo-con in a place free from low molecular siloxane.


### Operating Environment/Storage Environment

#### ⚠ Warning

##### 4. Installation conditions

If the space for the intake and discharge of air is insufficient, the amount of transferred air will decrease, which can impair the performance and life of the product. Therefore, keep the conditions illustrated below for installation. Also, if ambient temperature is expected to be over 35°C, vent or exhaust air to prevent the increase of ambient temperature over 35°C.

<HEC006/012>



<HEC001/003>

It is not necessary to leave space for ventilation. Install the product while taking working space for installation and maintenance into account. However, ventilation must be also considered so that ambient temperature does not excessively rise.

### Facility Water

#### ⚠ Caution

##### 1. If the temperature of the facility water is too low, it can cause formation of dew condensation inside the heat exchanger.

Supply facility water with a temperature over the atmospheric dew point to avoid the formation of dew condensation.

##### 2. If the facility water piping is connected to multiple machines, the facility water exchanges heat at the upstream side and its temperature will become higher as it goes downstream.

Limit the number of connected Thermo-cons to two per facility water system, and if more than two Thermo-cons are to be connected, increase the number of systems.

### Circulating Fluid

#### ⚠ Caution

##### 1. Use tap water or fluid which will not damage the wetted parts material as described in this catalog's specifications.

(PPE, PP glass 10%, Alumina ceramics, Carbon, EPDM, Stainless steel 303, Stainless steel 304, PE, PP, NBR)

##### 2. Deionized water (with an electrical conductivity of approx. 1 µS/cm) can be used, but may lose its electrical conductivity.



# Series HEC-W

## Specific Product Precautions 2

Be sure to read this before handling. Refer to front matter 41 for Safety Instructions and pages 1246 to 1249 for Temperature Control Equipment Precautions.

### Circulating Fluid

#### Caution

3. If deionized water is used, bacteria and algae may grow in a short period.

If the Thermo-con is operated with bacteria and algae, its heat exchanging capacity or the capacity of the pump may deteriorate. Exchange all deionized water regularly depending on the conditions (once a month as a guide).

4. If using a fluid other than this catalog, please contact SMC beforehand.

5. The maximum operating pressure of circulating fluid circuit is 0.1 MPa.

If this pressure is exceeded, leakage from the tank in the Thermo-con can result.

6. Select a pipe with a length and diameter which allow a flow rate of 3 L/min or more for the circulating fluid.

If the flow rate is less than 3 L/min, the Thermo-con cannot provide precise control, but also can fail because of the repeated cooling and heating operation.

7. A magnet driven pump is used as a circulating pump.

A fluid which contains metal powders such as iron powder cannot be used.

8. The Thermo-con must not be operated without circulating fluid.

The pump can break due to idling.

9. If the tank lid is opened after the supply of circulating fluid, the circulating fluid may spill out depending on the condition of external piping.

10. If an external tank is used, the circulating fluid may spill out from the internal tank lid depending on where the external tank is installed.

Check that the internal tank has no leakage if using an external tank.

11. If there is a point where fluid is released to atmosphere externally (tank or piping), minimize the piping resistance at the circulating fluid return side.

If the piping resistance is too large, the piping may be crushed, or the built-in circulator tank may be deformed or cracked because the pressure in the piping for return will become negative. The built-in circulator tank is made of resin (PE). Therefore, the tank may be crushed if the pressure is negative. Special attention must be paid if the flow rate of the circulating fluid is high. To avoid getting negative pressure less than -0.02 MPa, the piping for return should be as thick and short as possible to minimize the piping resistance. It is also effective to restrict the flow rate of circulating fluid or remove the gasket of internal tank for the release to atmosphere.

12. If fluorinated fluid is used in the Thermo-con (HEC006/012), static electricity will be generated by the flow of fluid. This static electricity may be discharged to the board of the Thermo-con, causing damage or operation failure and loss of data of such as set temperature.

Ground pipe in order to remove static electricity.

13. Avoid operation with cavitation or bubbles due to low fluid level in the tank. This may shorten the pump life.

### Circulating Fluid

#### Caution

14. If clear water is used, it should satisfy the quality standards shown below.

#### Clear Water (as Circulating Water) Quality Standards

The Japan Refrigeration and Air Conditioning Industry Association  
JRA GL-02-1994 "Cooling water system - Circulating type - Supply water"

	Item	Unit	Standard value	Influence	
				Corrosion	Scale generation
Standard Item	pH (at 25°C)	—	6.0 to 8.0	○	○
	Electrical conductivity (25°C)	[μS/cm]	100* to 300*	○	○
	Chloride ion (Cl <sup>-</sup> )	[mg/L]	50 or less	○	
	Sulfuric acid ion (SO <sub>4</sub> <sup>2-</sup> )	[mg/L]	50 or less	○	
	Acid consumption amount (at pH4.8)	[mg/L]	50 or less		○
	Total hardness	[mg/L]	70 or less		○
	Calcium hardness (CaCO <sub>3</sub> )	[mg/L]	50 or less		○
	Ionic state silica (SiO <sub>2</sub> )	[mg/L]	30 or less		○
Reference Item	Iron (Fe)	[mg/L]	0.3 or less	○	○
	Copper (Cu)	[mg/L]	0.1 or less	○	
	Sulfide ion (S <sub>2</sub> <sup>-</sup> )	[mg/L]	Should not be detected.	○	
	Ammonium ion (NH <sub>4</sub> <sup>+</sup> )	[mg/L]	0.1 or less	○	
	Residual chlorine (Cl)	[mg/L]	0.3 or less	○	
	Free carbon (CO <sub>2</sub> )	[mg/L]	4.0 or less	○	

\* In the case of [MΩ·cm], it will be 0.003 to 0.01.

○: Factors that have an effect on corrosion or scale generation.

• Even if the water quality standards are met, complete prevention of corrosion is not guaranteed.

### Communication

#### Caution

1. The set value can be written to EEPROM, but only up to approx. 1 million times.

In particular, pay attention to how many of times the writing is performed using the communication function.

### Maintenance

#### Warning

1. Prevention of electric shock and fire

Do not operate the switch with wet hands. Also, do not operate the Thermo-con with water left on it.

2. Action in the case of error

If any error such as abnormal sounds, smoke, or bad smell occurs, cut off the power at once, and stop supplying and conveying fluid. Please contact SMC or a sales distributor to repair the Thermo-con.

3. Regular inspection

Check the following items at least once a month. The inspection must be done by an operator who has sufficient knowledge and experience.

- Check of displayed contents.
- Check of temperature, vibration and abnormal sounds in the body of the Thermo-con.
- Check of the voltage and current of the power supply system.
- Check for leakage and contamination of the circulating fluid and intrusion of foreign objects to it, and subsequent replacement of water.
- Check for leakage, quality change, flow rate and temperature of facility water.